

Smart Medical Accurate Finger Pulse Oximeter Wireless Blood Oxygen Monitor

Basic Information

- Place of Origin:
- Brand Name:
- ΗY CE/CFDA/RoHs/FCC/ISO13485/FDA • Certification: HY-02

China

- Model Number:
- Minimum Order Quantity: 200PCS
- Price: 8~12USD
- Packaging Details:

🔊 accurate



Product Specification

- Type:
- Fingertip Pulse Oximeter
- Instrument Classification:
- Color:
- Function:
- Feature:
- Highlight:
- Class II

OPP packing , 200pcs Per Carton

- Black/White/Pink/Blue
- Measure PR, SpO2
- LED/TFT/OLED ,Easy To Carry
 - Medical Accurate Finger Pulse Oximeter, Smart Accurate Finger Pulse Oximeter, Wireless Blood Oxygen Monitor

Wireless Blood Oxygen Monitor With Audio Reminder On Device & Smart Medical Pulse Oximeter

Why have I been told to use a pulse oximeter?

You may have been told by your doctor to use a pulse oximeter because you are recovering from COVID-19, or because you are a patient who is at higher risk of suffering with COVID-19. Using a pulse oximeter is a good way of making sure your breathing levels aren't worsening.



Intelligent Voice Prompt

There is a pulse beep during measurement. When the blood oxygen value and heart rate value are abnormal, the screen flashes and a beep tone sounds





Turn off/on the sound: long press the power button for 2 seconds to turn off/on the sound. No need to keep pressing, just 2 seconds!

Caution:

The finger should be placed properly; else, the provided results could be inaccurate.

The photoelectric receiving tube and the SpO2 sensor must be arranged in accordance with the subject's arteriole position.

The SpO2 sensor shouldn't be applied at a location or limb linked with arterial canal or blood pressure cuff or receiving an intravenous injection.

Keep the optical path free from any optical like rubberized fabric.

Refrain excessive ambient lighting such as an infrared heater, direct sunlight, fluorescent lamp, dual ruby light, etc., for protecting it from affecting the measuring results.

Strenuous action of the subject or extreme electrosurgical interference can affect the accuracy.

Testee cannot use enamel or other makeup.

Operating Guide:

Batteries must be inserted in the proper direction and then replaced by the cover.

The clip must be open as visualized below. The finger must be placed in a proper position.

The patient's finger must be placed aligned with the clip's rubber cushions in the right position and then clip the finger.

The switch on the front panel should be pressed.

During the process, the patient should be kept stationary and avoid the finger from shaking.

Information is presented directly on the screen display.

Repairing and Maintenance:

If there is a low-voltage warning, change the batteries.

Use alcohol swaps to clean the device always before using and then let it fry or clean it until dry with a clean fabric.

Medical alcohol should be applied for disinfecting the product and preventing it from being infected the next time.

Take out the batteries if you're not going to use the oximeter for a long time.

Ideal temperatures are 40°C to 60°C, and the humidity should be kept below 95%.

The device needs to be calibrated once a year (or according to the hospital's calibrating program). It also can be performed at the stateappointed agent or contact us for calibration.

Specification:

for more products please visit us on oxygenconcentratormedical.com

Dimension: 60mm×35mm×32mm

Weight: 50g

SPO2 Range: 0% - 99%.

SPO2 Resolution: +- 1%.

Pulse Rate Range: 30-250 bpm.

Pulse Rate Resolution: +- 1bpm.

Power Requirements: 2 ×1.5V AAA alkaline battery or rechargeable battery instead, adaptable range: 2.6V~3.6V.

Measurement Performance: Oxyhemoglobin/Pulse value is accurate when the pulse-filling rate is 0.4%.

The deviation is smaller than +- 1 % when measured in natural indoor lighting conditions.

One size fits all


Package Contents:

1*Pulse Oximeter

1*One hanging rope

1*User Manual

1*Storage bag

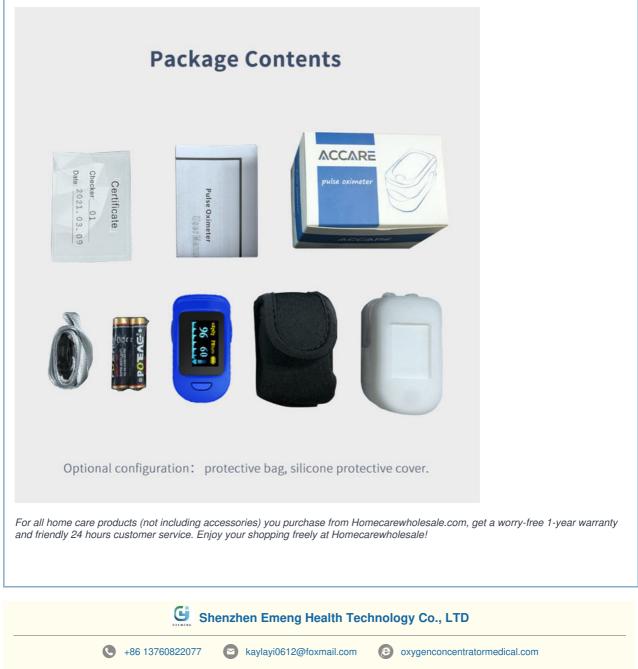

Room D, 7th Floor, Guang Long Building, 162 Ping Xin North Road, PingHu Street, LongGang District, ShenZhen