

## 8mins Test Time Best 9 IN1 Multiplex Respiratory Test Kit for Fast and Accurate Results

Our Product Introduction

for more products please visit us on [oxygenconcentratormedical.com](http://oxygenconcentratormedical.com)

### Basic Information

- Place of Origin: China
- Brand Name: DVOT
- Certification: CE/ISO
- Model Number: 9 in1
- Minimum Order Quantity: 360 test
- Price: 2.4USD
- Packaging Details: QTY: 360T/PER CTN; Weight :14KGS; CTN SIZE : 46\*44\*44CM
- Delivery Time: 15-20 work days
- Payment Terms: D/P, T/T, Western Union, MoneyGram
- Supply Ability: 1000000pcs



### Product Specification

- Test Time: 8mins
- Time Of Use: Disposable
- Keyword: Antigen Rapid Test
- Date Of Use: 1.5 Years
- Highlight: 9 IN1 Multiplex Respiratory Test Kit , Fast Multiplex Respiratory Test Kit , Accurate Multiplex Respiratory Test Kit



### More Images



## Product Description

### Best At-home Flu and 9 IN1 Multiplex Respiratory Test Kit for Fast Tests with high accuracy

#### Product Description:

During the first few days of a new coronavirus infection, symptoms are often nonspecific and may include cough, fever, and sore throat. These symptoms can be difficult to distinguish from other viral infections such as influenza, respiratory syncytial virus (RSV) or viruses associated with the common cold.

DOVT's Multiple Respiratory Antigen Test is designed to detect if your symptoms are caused by one of the following viruses: SARS-COV-2 & RSV & MP & ADV & Flu AB & PIV1/3 & PIV2 & HMPV. When a combined diagnostic is performed to determine the cause of the disease, the appropriateness of treatment can be determined, and targeted therapy can be administered.

In summary, the Multiplex Respiratory Antigen Test Kit allows you to quickly determine which infections are causing symptoms and does not require rigorous training, but can be used anywhere, anytime by following the instructions.

#### Advantage:

- ✓ Get results at home
- ✓ Self-testing made easy
- ✓ Save time
- ✓ Results in 8 minutes
- ✓ Can be stored for a long time
- ✓ Simple testing procedure

Test Time	8mins
Time Of Use	Disposable
Keyword	Antigen Rapid Test
Date of use	1.5 years

#### Support and Services:

**Our medical diagnostic test kits are designed for accuracy and ease of use. We offer technical support services to assist with any questions or issues that may arise during the testing process.**

**Our goal is to provide our customers with the highest level of support and service to ensure successful testing outcomes.**

# Infected or not? Test right now!



## Multiplex Respiratory Antigen Test Kit

**New**  
**Omicron**  
EG.5.CH.1.1 JN-1  
Detected

SARS-CoV-2 | RSV | MP | ADV | Flu A/B | PIV 1/3 | PIV 2 | HMPV

**9 In 1**



Anterior **Nasal** Swab  
Anteriorer Nasenabstrich

SARS-CoV-2 **94.55%**  
Sensitivity

Influenza A **90.48%**  
Sensitivity

Influenza B **91.67%**  
Sensitivity

RSV **93.62%**  
Sensitivity



MP **90.82%**  
Sensitivity

ADV **91.18%**  
Sensitivity

PIV1/3 **92.23%**  
Sensitivity

PIV2 **90.20%**  
Sensitivity

HMPV **90.6%**  
Sensitivity



### About the Antigen Combo Test Kit

During the first few days of a Covid-19 illness, symptoms tend to be nonspecific and may include cough, fever and sore throat. These symptoms can be indistinguishable from other viral infections, such as influenza, respiratory syncytial virus (RSV), or viruses associated with the common cold. Because of this, combo diagnostic testing is needed and important, not only to determine the cause of the illness, but also to determine whether treatment is appropriate.

SARS-CoV-2 & RSV & MP & ADV & Flu A/B & PIV1/3 & PIV2 & HMPV Antigen Combo Test Kit is an easy and rapid way to identify which infections cause the symptoms. It can be used anywhere and anytime by yourself.



Get result at home



Easy self-testing



Time-saving

**Anytime, Anywhere, Test by yourself !**



Hospital



Test Site



Airport



Station



Hotel



Corporation



Mass Screening

## HAVE YOU EVER HAD SUCH CONCERNS?

### Worried about inconvenient to test

- No hospitals or test site available nearby.
- Physical discomfort, queue for a long time to test.

### Worried about can not get result immediately

- Long time waiting for a PCR test result.
- Want to know the result immediately.

### Worried about the family

- Anyone in my family been infected?
- How to test elder and infants?

### Worried about infection

- Infection risk in crowded hospitals or test site.
- If there are close contacts around you?



Let us  
**SOLVE**  
your troubles!

It can detect mutated virus

## High accuracy detection $\geq 96\%$

- ✓ Test result is available in 8 minutes.
- ✓ Self-testing is convenient at home, or anywhere else.
- ✓ Risk control for easy life and working.
- ✓ Shelf-life of 1.5 years, you can store for a long time.


Easy detection will make you feel ease, people around you also feel comfortable.

## Simple steps, easy-handling for anybody!





## Result Reading

### For Cov & Rsv

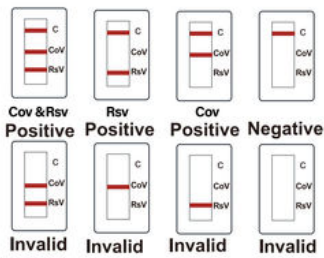

### For MP & ADV & HMPV

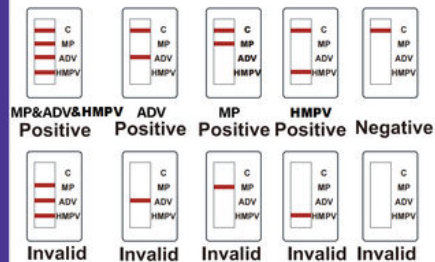

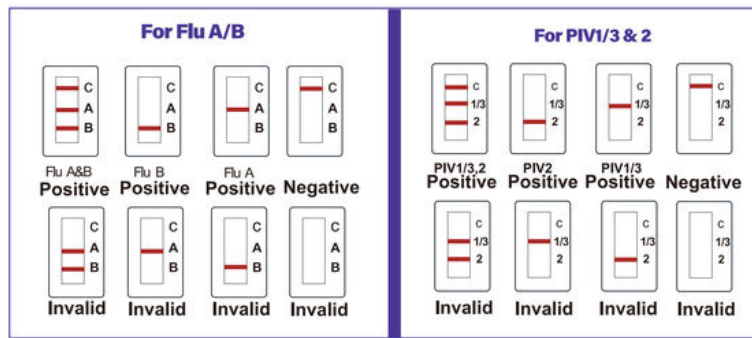



## Shipping Details



CB	
QTY :	360 PCS
G.W :	14 KG
MEAS :	46X44X44CM




**QUICK USER GUIDE**

**9 In 1** 

使用說明書  
**多項呼吸病毒檢體快速測試盒**  
多項呼吸病毒快速測試盒

2. 分鐘快速檢結果

2. 分鐘快速檢結果, 檢出結果可即時顯示



**9 In 1**

**Multiplex Assay for Use**

**Multiple Respiratory Antigen Test Kit**

BARCELONA 10-16-17-18-19-20-21-22-23-24-25-26-27-28-29-30-31-32-33-34-35-36-37-38-39-40-41-42-43-44-45-46-47-48-49-50-51-52-53-54-55-56-57-58-59-60-61-62-63-64-65-66-67-68-69-70-71-72-73-74-75-76-77-78-79-80-81-82-83-84-85-86-87-88-89-90-91-92-93-94-95-96-97-98-99-100-101-102-103-104-105-106-107-108-109-110-111-112-113-114-115-116-117-118-119-120-121-122-123-124-125-126-127-128-129-130-131-132-133-134-135-136-137-138-139-140-141-142-143-144-145-146-147-148-149-150-151-152-153-154-155-156-157-158-159-160-161-162-163-164-165-166-167-168-169-170-171-172-173-174-175-176-177-178-179-180-181-182-183-184-185-186-187-188-189-190-191-192-193-194-195-196-197-198-199-200-201-202-203-204-205-206-207-208-209-210-211-212-213-214-215-216-217-218-219-220-221-222-223-224-225-226-227-228-229-230-231-232-233-234-235-236-237-238-239-240-241-242-243-244-245-246-247-248-249-250-251-252-253-254-255-256-257-258-259-260-261-262-263-264-265-266-267-268-269-270-271-272-273-274-275-276-277-278-279-280-281-282-283-284-285-286-287-288-289-290-291-292-293-294-295-296-297-298-299-300-301-302-303-304-305-306-307-308-309-310-311-312-313-314-315-316-317-318-319-320-321-322-323-324-325-326-327-328-329-330-331-332-333-334-335-336-337-338-339-340-341-342-343-344-345-346-347-348-349-350-351-352-353-354-355-356-357-358-359-360-361-362-363-364-365-366-367-368-369-370-371-372-373-374-375-376-377-378-379-380-381-382-383-384-385-386-387-388-389-390-391-392-393-394-395-396-397-398-399-400-401-402-403-404-405-406-407-408-409-410-411-412-413-414-415-416-417-418-419-420-421-422-423-424-425-426-427-428-429-430-431-432-433-434-435-436-437-438-439-440-441-442-443-444-445-446-447-448-449-450-451-452-453-454-455-456-457-458-459-460-461-462-463-464-465-466-467-468-469-470-471-472-473-474-475-476-477-478-479-480-481-482-483-484-485-486-487-488-489-490-491-492-493-494-495-496-497-498-499-500-501-502-503-504-505-506-507-508-509-510-511-512-513-514-515-516-517-518-519-520-521-522-523-524-525-526-527-528-529-530-531-532-533-534-535-536-537-538-539-540-541-542-543-544-545-546-547-548-549-550-551-552-553-554-555-556-557-558-559-560-561-562-563-564-565-566-567-568-569-570-571-572-573-574-575-576-577-578-579-580-581-582-583-584-585-586-587-588-589-590-591-592-593-594-595-596-597-598-599-600-601-602-603-604-605-606-607-608-609-610-611-612-613-614-615-616-617-618-619-620-621-622-623-624-625-626-627-628-629-630-631-632-633-634-635-636-637-638-639-640-641-642-643-644-645-646-647-648-649-650-651-652-653-654-655-656-657-658-659-660-661-662-663-664-665-666-667-668-669-670-671-672-673-674-675-676-677-678-679-680-681-682-683-684-685-686-687-688-689-690-691-692-693-694-695-696-697-698-699-700-701-702-703-704-705-706-707-708-709-710-711-712-713-714-715-716-717-718-719-720-721-722-723-724-725-726-727-728-729-730-731-732-733-734-735-736-737-738-739-740-741-742-743-744-745-746-747-748-749-750-751-752-753-754-755-756-757-758-759-760-761-762-763-764-765-766-767-768-769-770-771-772-773-774-775-776-777-778-779-780-781-782-783-784-785-786-787-788-789-790-791-792-793-794-795-796-797-798-799-800-801-802-803-804-805-806-807-808-809-810-811-812-813-814-815-816-817-818-819-820-821-822-823-824-825-826-827-828-829-830-831-832-833-834-835-836-837-838-839-840-841-842-843-844-845-846-847-848-849-850-851-852-853-854-855-856-857-858-859-860-861-862-863-864-865-866-867-868-869-870-871-872-873-874-875-876-877-878-879-880-881-882-883-884-885-886-887-888-889-890-891-892-893-894-895-896-897-898-899-900-901-902-903-904-905-906-907-908-909-910-911-912-913-914-915-916-917-918-919-920-921-922-923-924-925-926-927-928-929-930-931-932-933-934-935-936-937-938-939-940-941-942-943-944-945-946-947-948-949-950-951-952-953-954-955-956-957-958-959-960-961-962-963-964-965-966-967-968-969-970-971-972-973-974-975-976-977-978-979-980-981-982-98

### For PIV1&2

**PIV1&2**  
 Positive

**PIV2**  
 Positive

**PIV1&2**  
 Negative

**Interpretation**

The PIV1&2 is a reflexive A+ B100, SP+ A100, SP+ B100 (SP=SPIN) assay. It is a rapid, sensitive, and specific immunoassay for the detection of PIV1 and PIV2 antibodies in human serum. The assay is performed by adding a drop of the sample to the test well. A positive result is indicated by a color change from blue to red. A negative result is indicated by a color change from blue to yellow.

**Test Principle**

Design Control: Test kit is based on the principle of colorimetric immunoassay. The test kit contains a microplate with 96 wells. The test is performed by adding a drop of the sample to the test well. A positive result is indicated by a color change from blue to red. A negative result is indicated by a color change from blue to yellow.

**Materials Required but not Provided**

One Person (Positive Element)

**Storage and Stability**

Store at 2-8°C. Do not freeze. The test kit is stable for 12 months. The test kit is stable for 12 months.

**Test Limitations**

1. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
2. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
3. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
4. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
5. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
6. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
7. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
8. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
9. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.
10. The test is not intended for the diagnosis of PIV1 and PIV2 in patients with severe immunosuppression.

### Cross-reactivity and Microbial Interference

The immunoassay study and the visual inspection study, in accordance with the manufacturer's instructions, have shown that the test is specific for PIV1 and PIV2. The test is not cross-reactive with other pathogens. The test is not affected by microbial interference.

**For SARS-CoV-2**

Pathogen	Antibody	Antigen
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-CoV-2	Positive	Positive
SARS-CoV-2	Negative	Negative
SARS-CoV-2	Positive	Negative
SARS-CoV-2	Negative	Positive
SARS-Co		

